

FIG 1

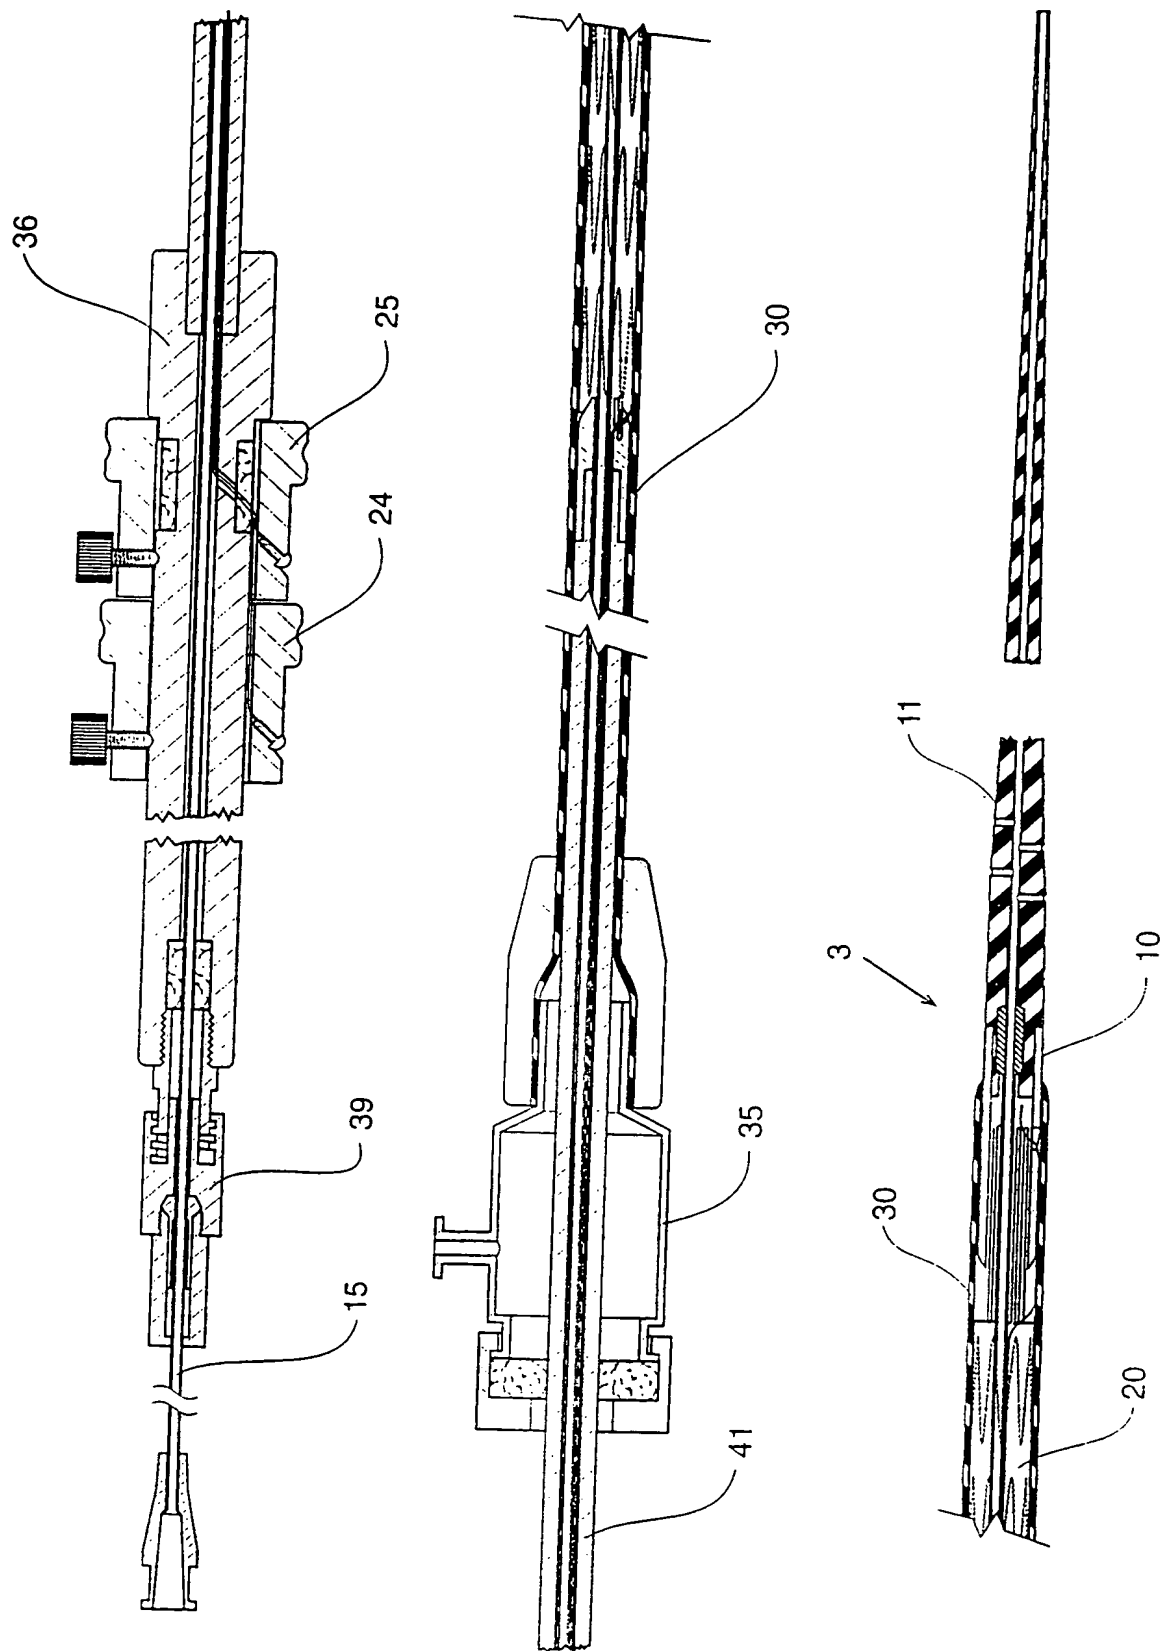


FIG 2

FIG 3

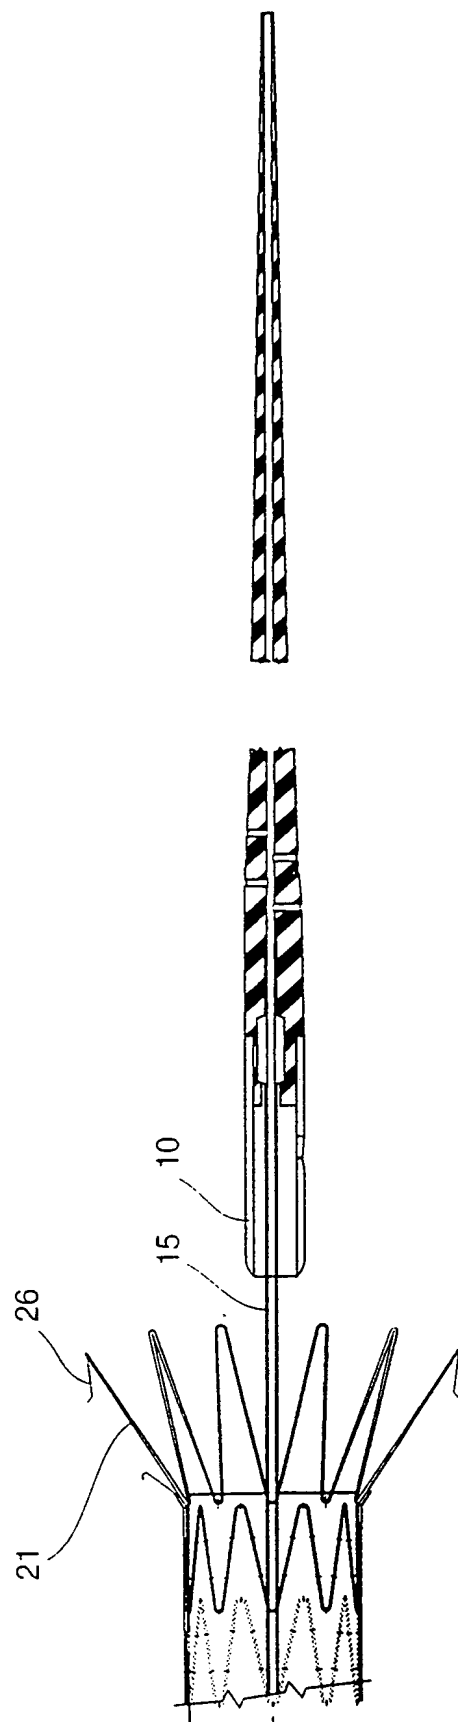
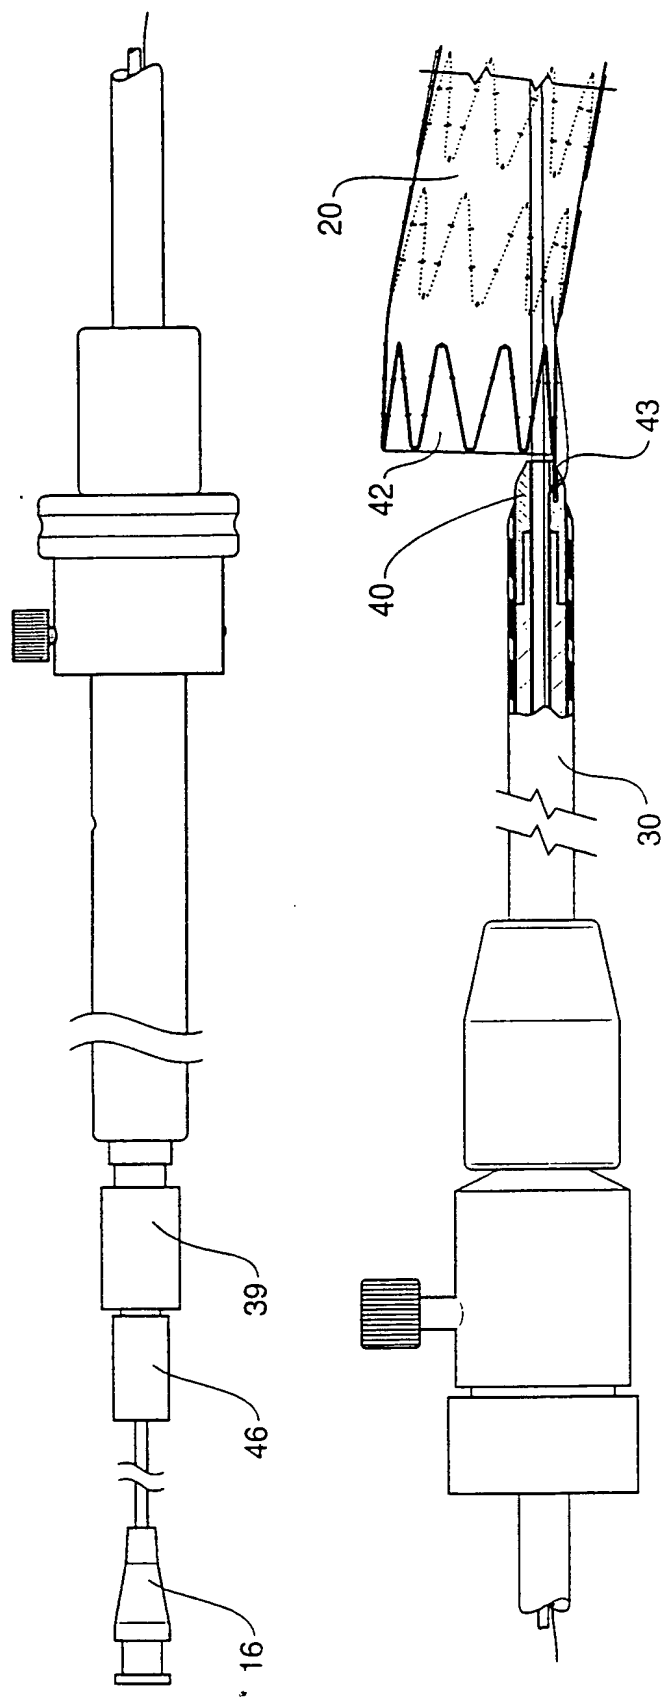


FIG 4

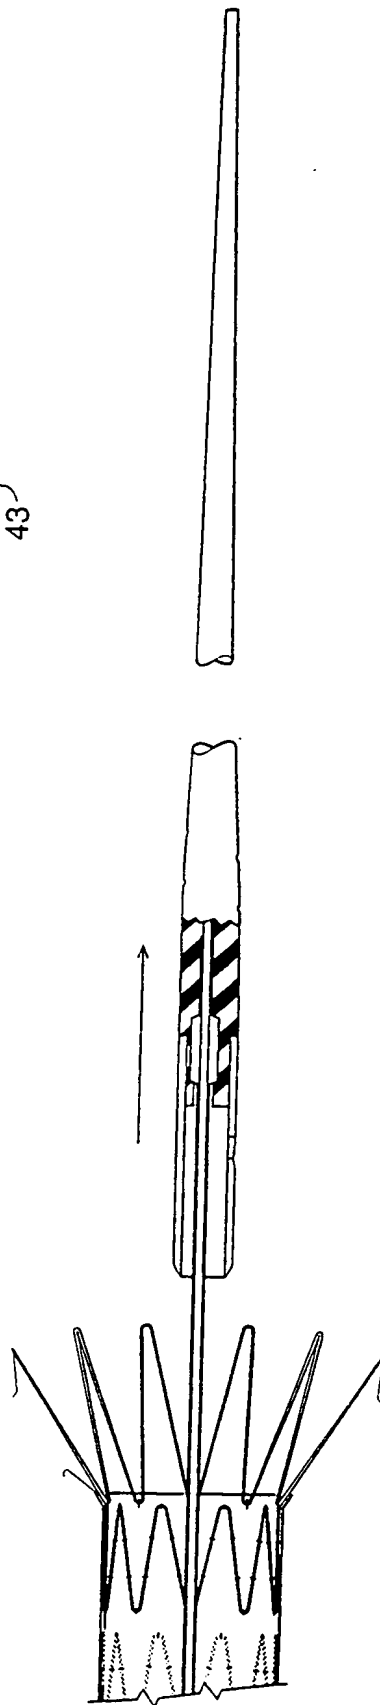
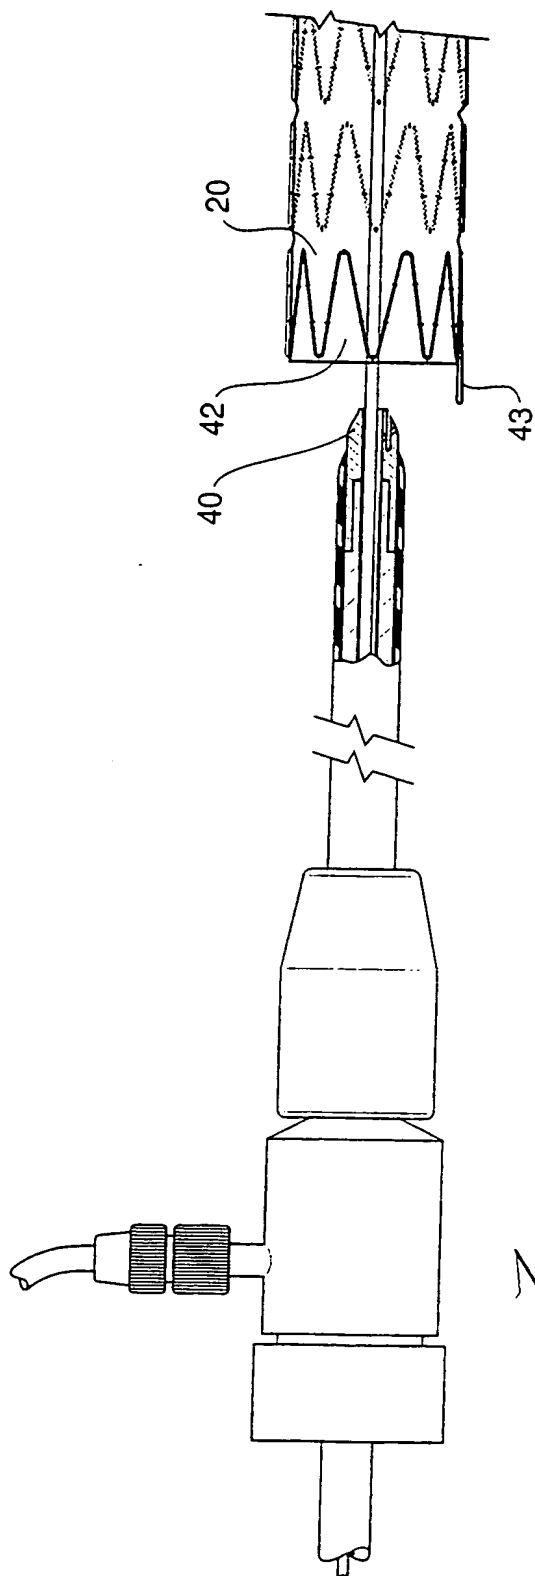
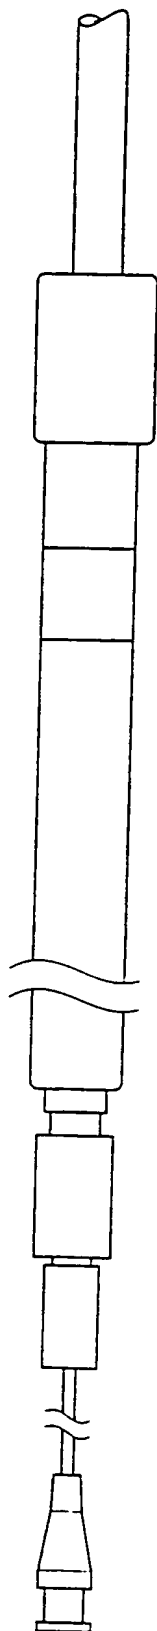


FIG 5

FIG. 6 is a schematic diagram of a cable assembly 100 in a first configuration. The cable assembly 100 includes a cable 102, a connector 104, and a plug 106. The cable 102 is connected to the connector 104, which is connected to the plug 106. The plug 106 is inserted into a port 108 of a device 110. The device 110 is shown in a perspective view.

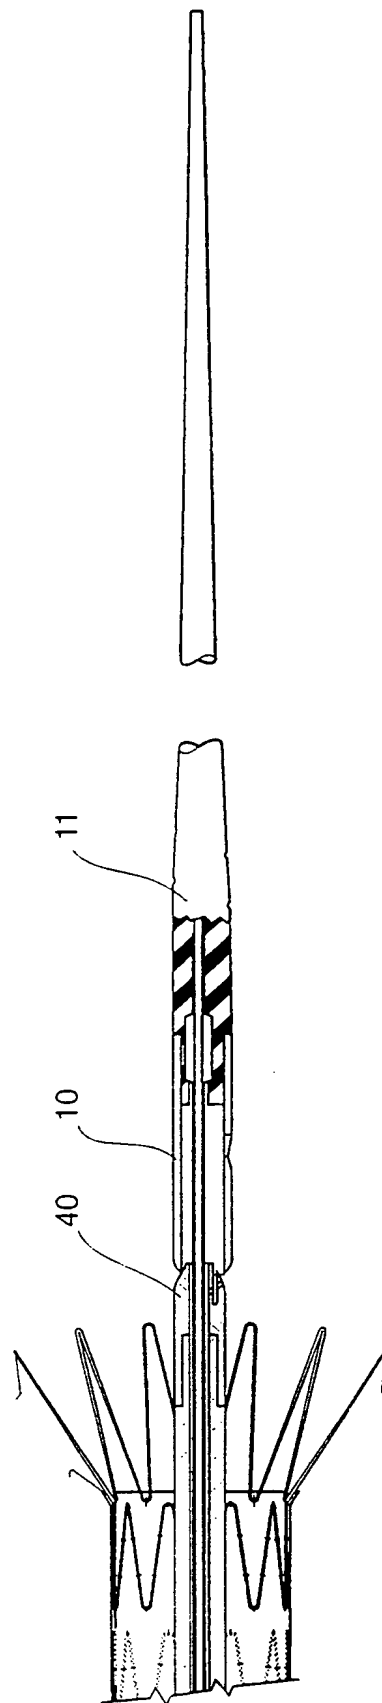
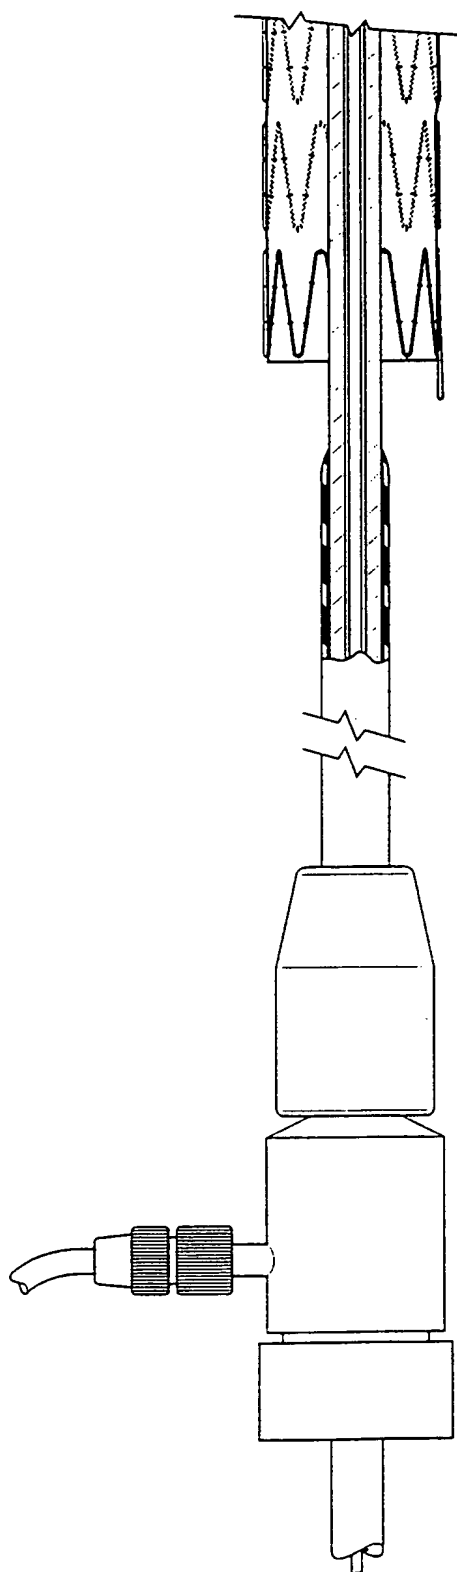
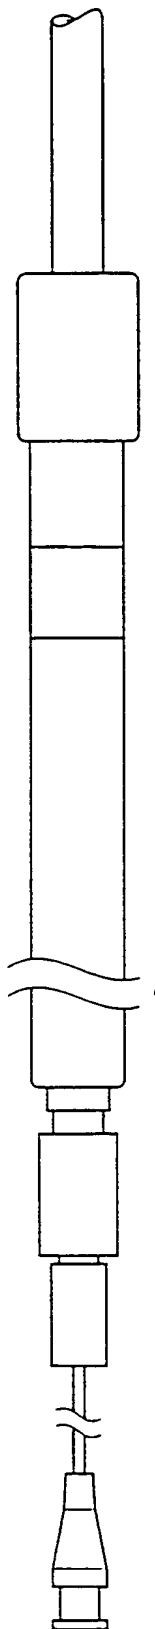


FIG 6

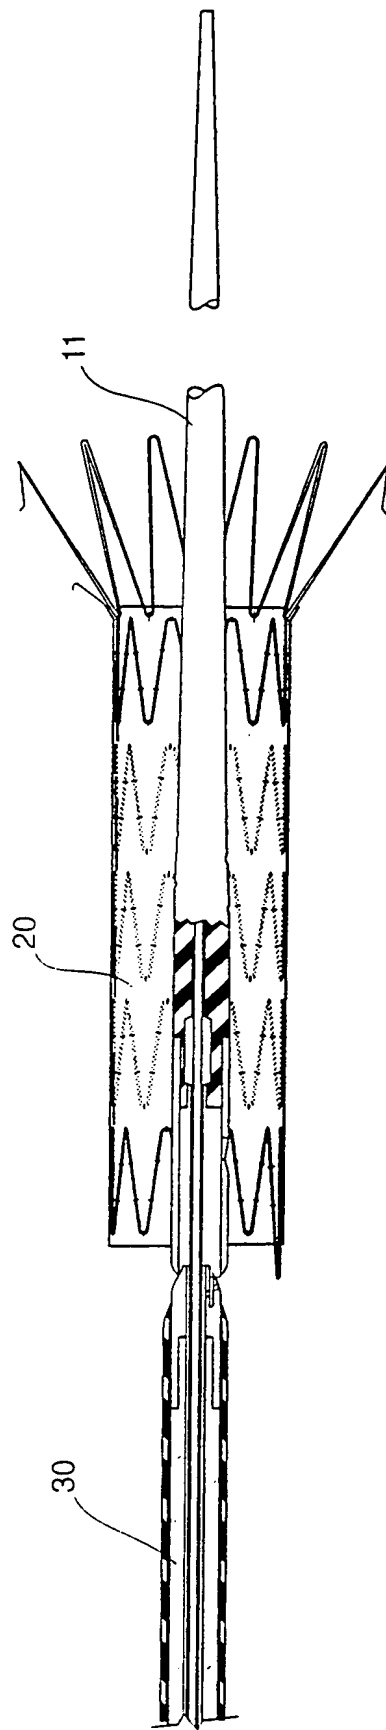
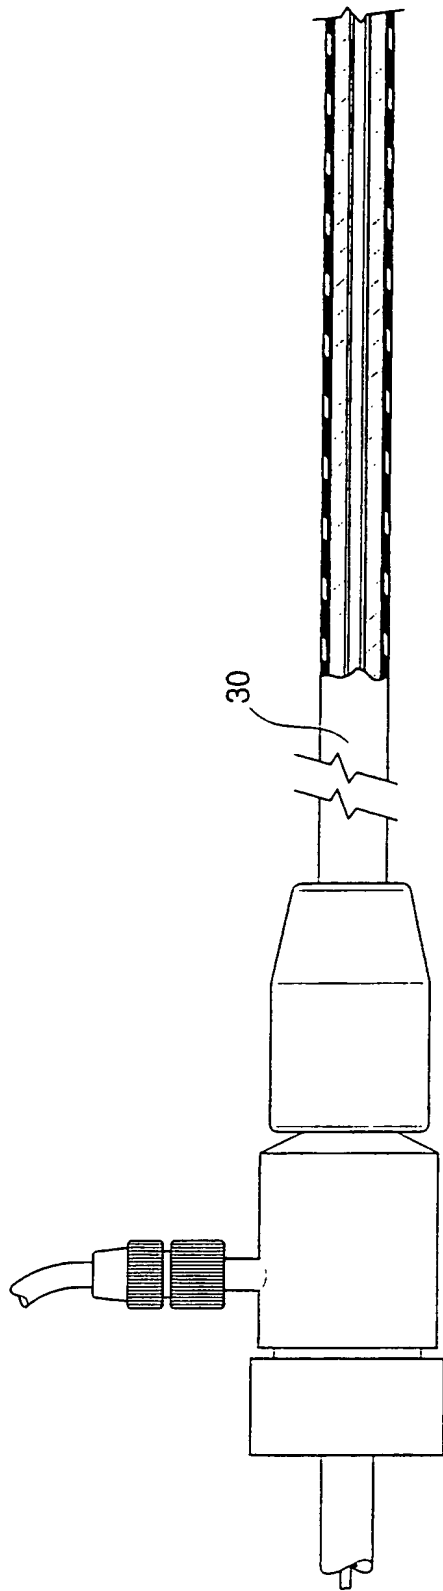
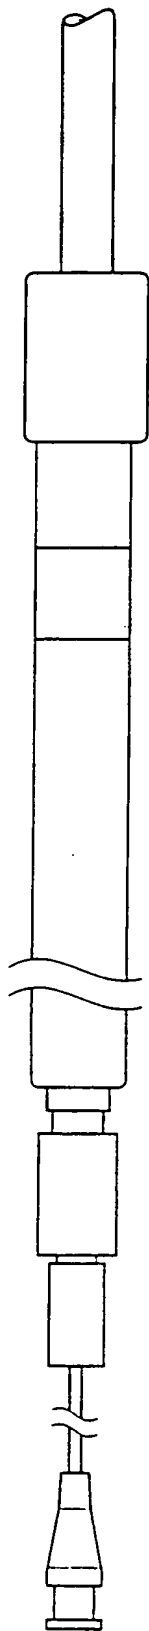


FIG 7

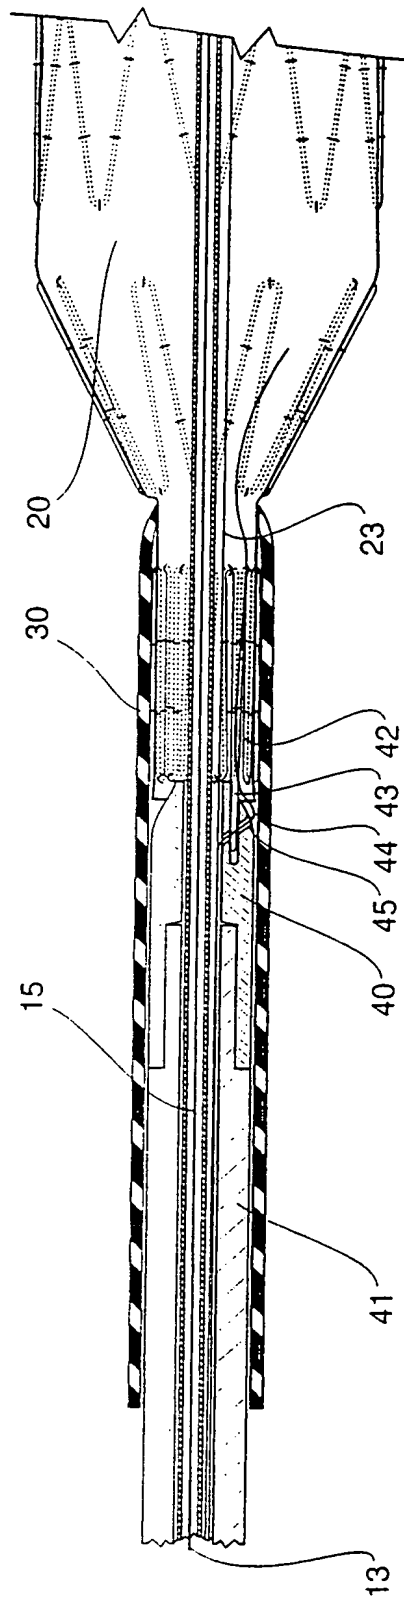


FIG 8

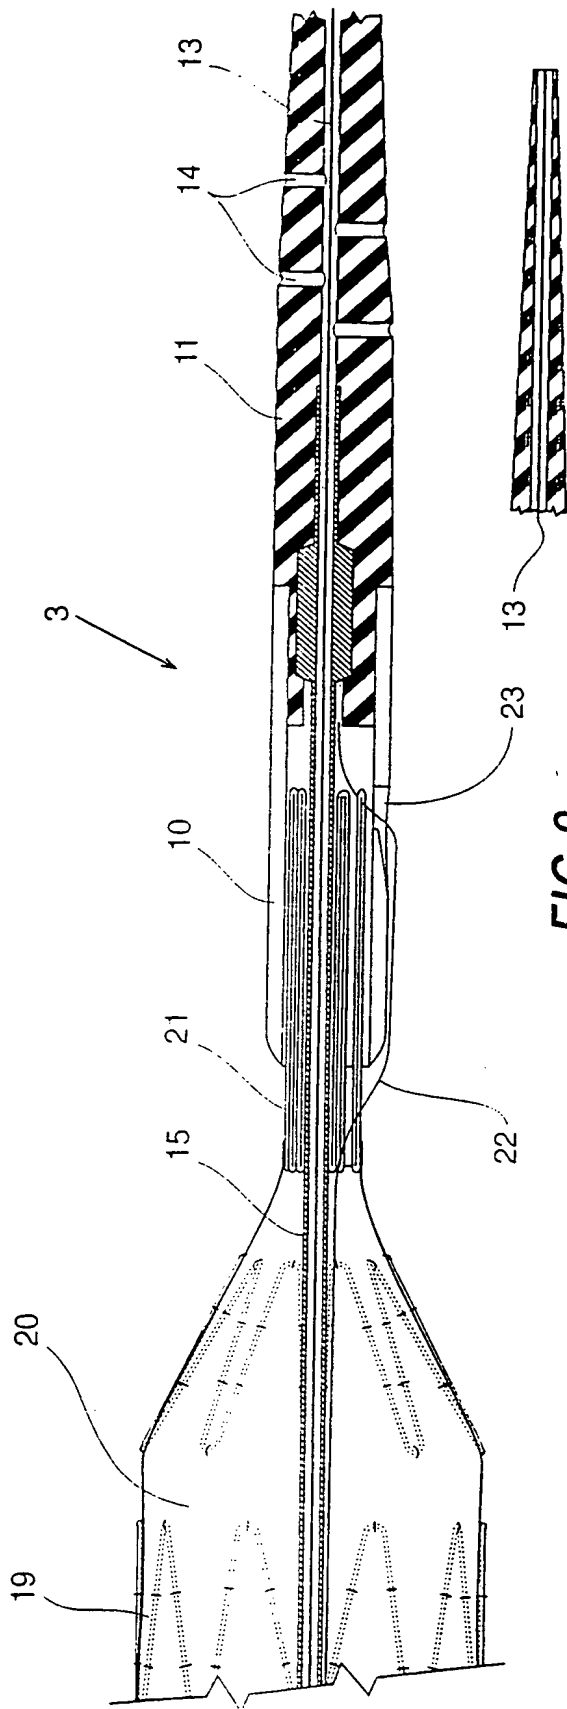


FIG 9

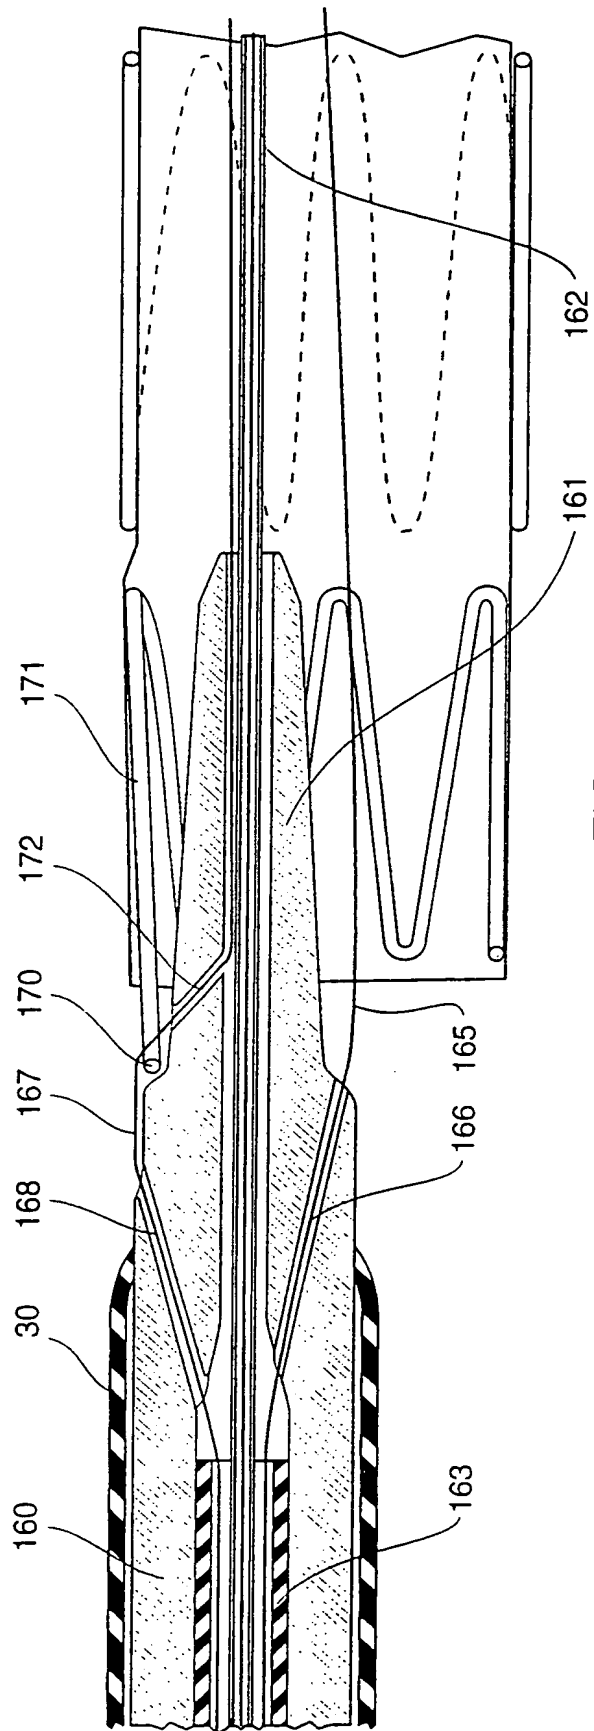


FIG. 8A

175

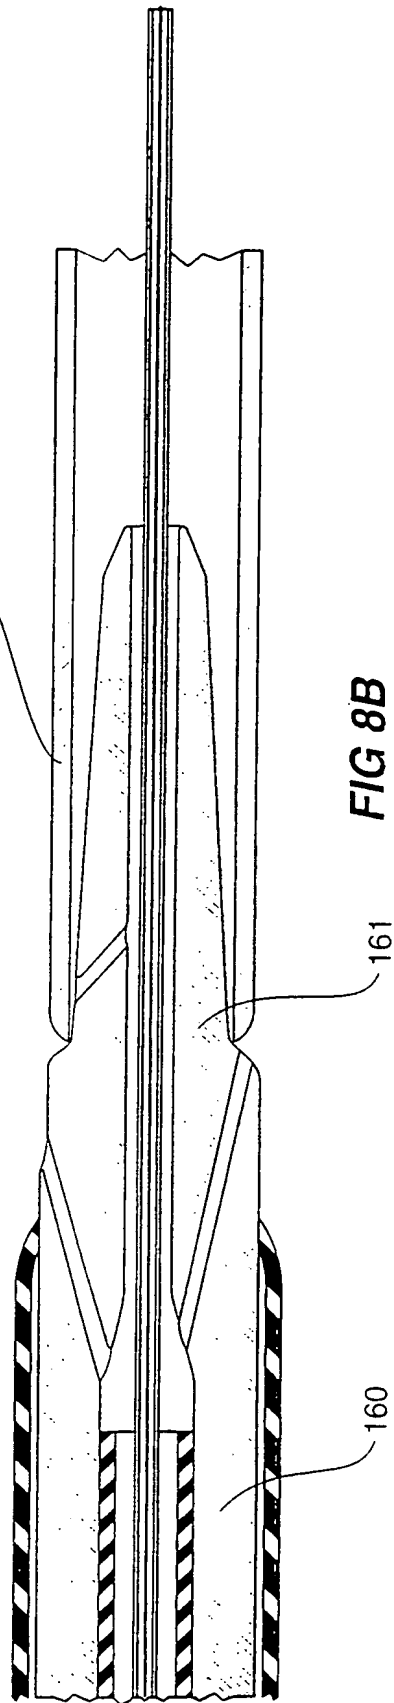


FIG. 8B

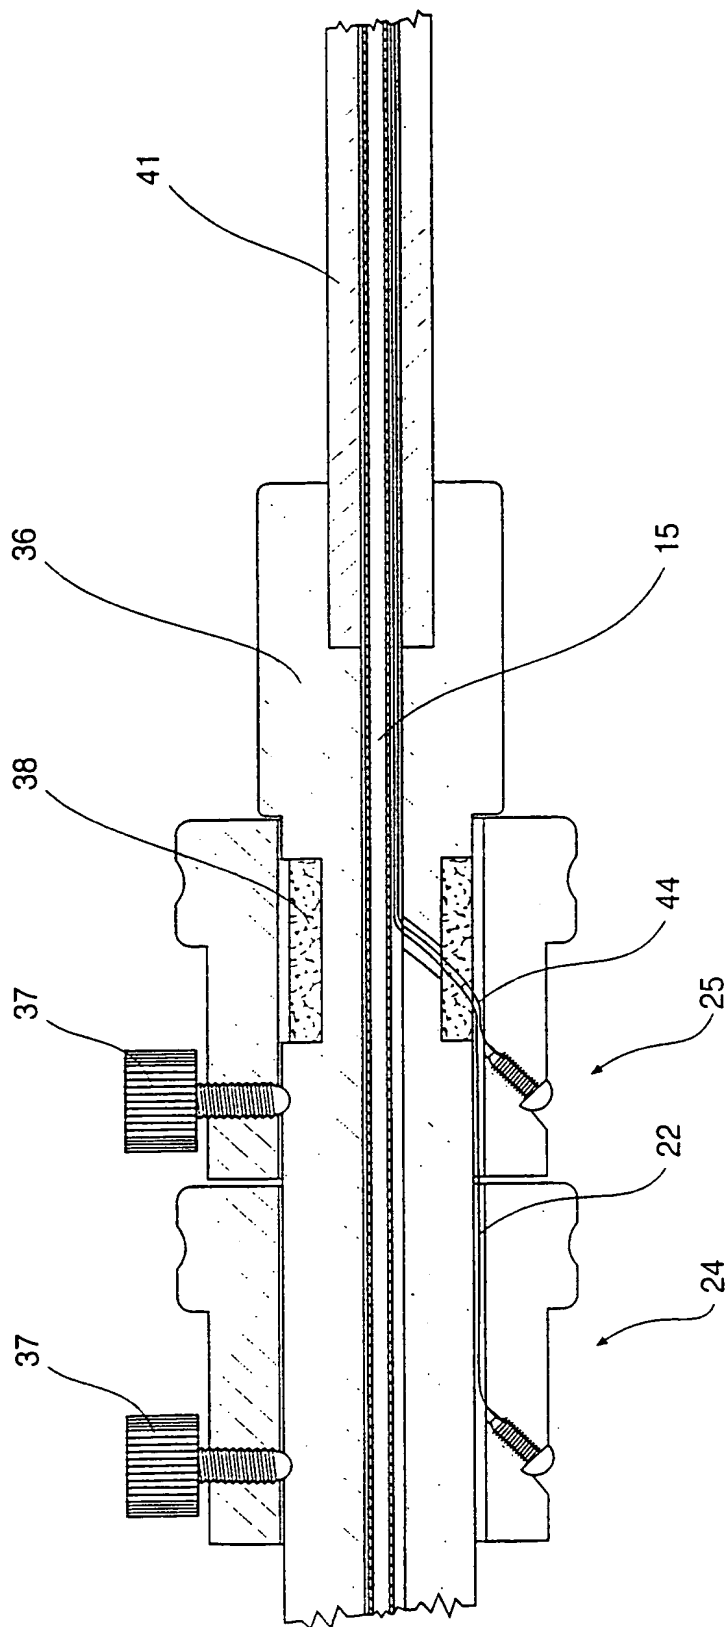


FIG 11

FIG. 13A is a cross-sectional view of a device 50 in a first state. The device 50 includes a central core 51 and a plurality of layers 52, 53, 54, 55, 56, 57, 58, 59, 60, 61, 62, 63, 64, 65, 66, 67, 68, 69, 70, 71, 72, 73, 74, 75, 76, 77, 78, 79, 80, 81, 82, 83, 84, 85, 86, 87, 88, 89, 90, 91, 92, 93, 94, 95, 96, 97, 98, 99, 100. The device 50 is shown in a cross-sectional view, with the central core 51 and the layers 52, 53, 54, 55, 56, 57, 58, 59, 60, 61, 62, 63, 64, 65, 66, 67, 68, 69, 70, 71, 72, 73, 74, 75, 76, 77, 78, 79, 80, 81, 82, 83, 84, 85, 86, 87, 88, 89, 90, 91, 92, 93, 94, 95, 96, 97, 98, 99, 100. The device 50 is shown in a cross-sectional view, with the central core 51 and the layers 52, 53, 54, 55, 56, 57, 58, 59, 60, 61, 62, 63, 64, 65, 66, 67, 68, 69, 70, 71, 72, 73, 74, 75, 76, 77, 78, 79, 80, 81, 82, 83, 84, 85, 86, 87, 88, 89, 90, 91, 92, 93, 94, 95, 96, 97, 98, 99, 100.

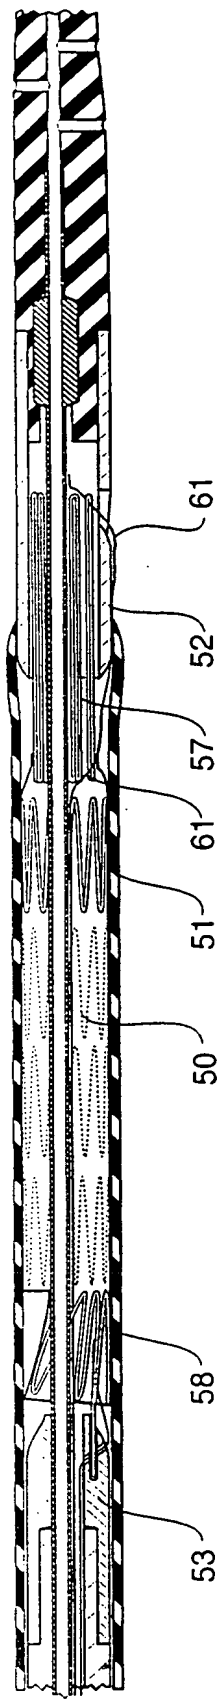


FIG 13A

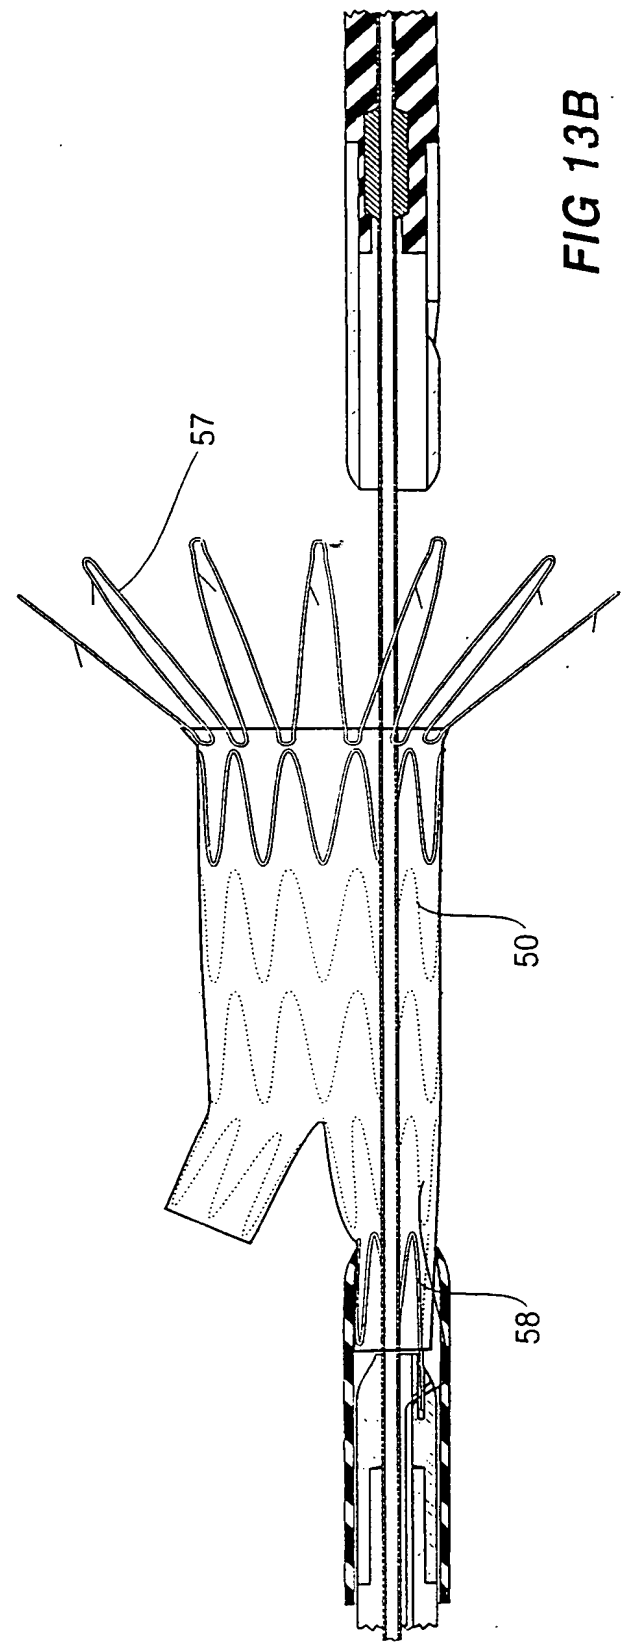


FIG 13B

FIG. 13C is a perspective view of the device 100 in a retracted position. The device 100 includes a handle 110, a shaft 120, and a distal tip 130. The handle 110 is connected to the shaft 120, which is connected to the distal tip 130. The distal tip 130 is shown in a retracted position, where it is folded back towards the handle 110. The device 100 is shown in a perspective view, with the handle 110, shaft 120, and distal tip 130 all visible. The device 100 is shown in a retracted position, where the distal tip 130 is folded back towards the handle 110.

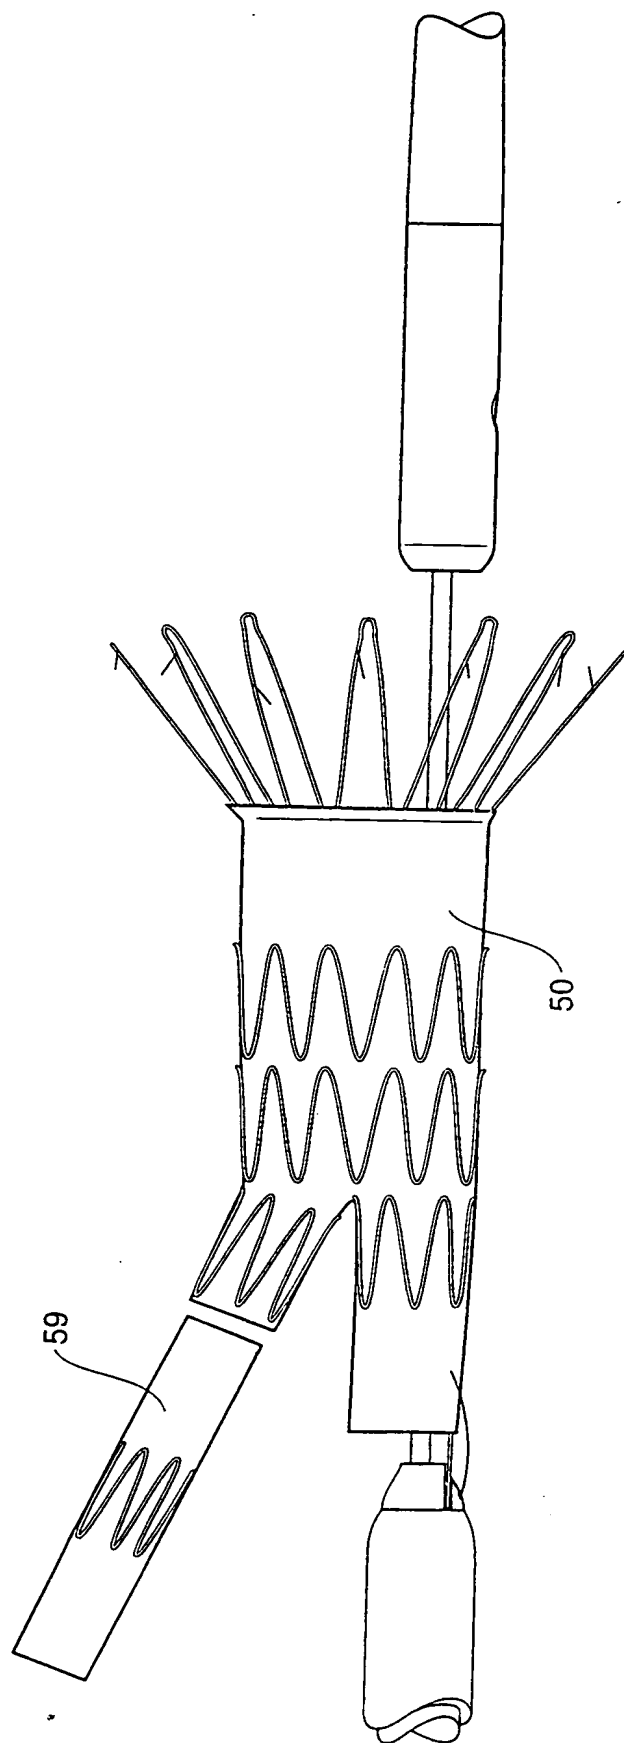


FIG 13C

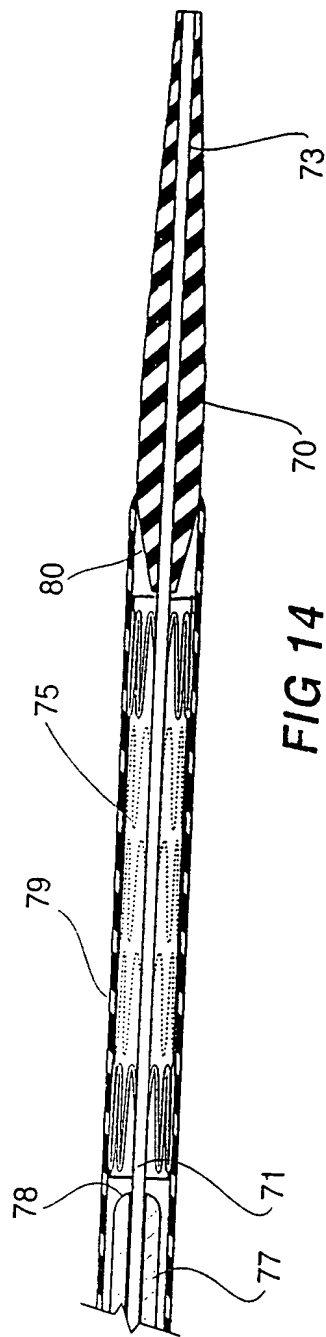
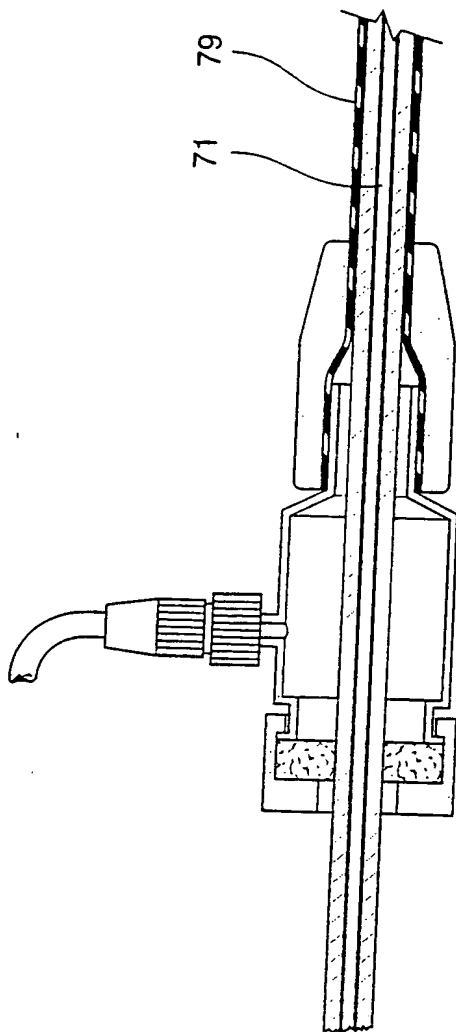
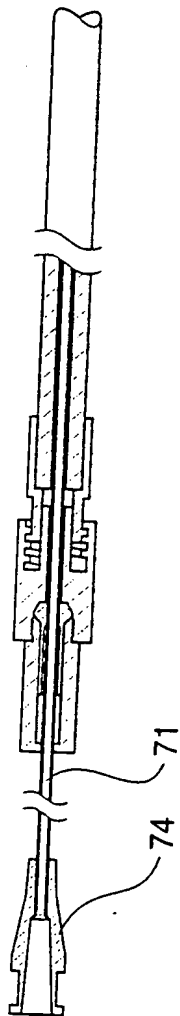


FIG 14

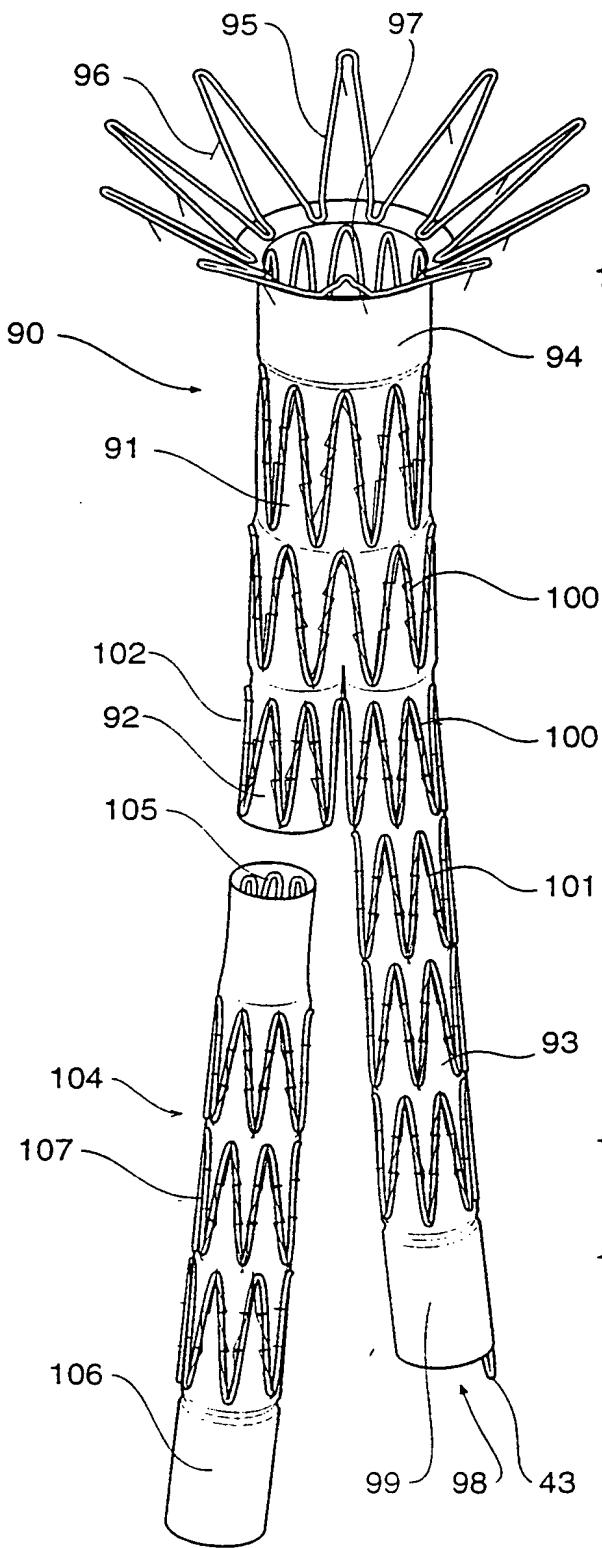


FIG 15

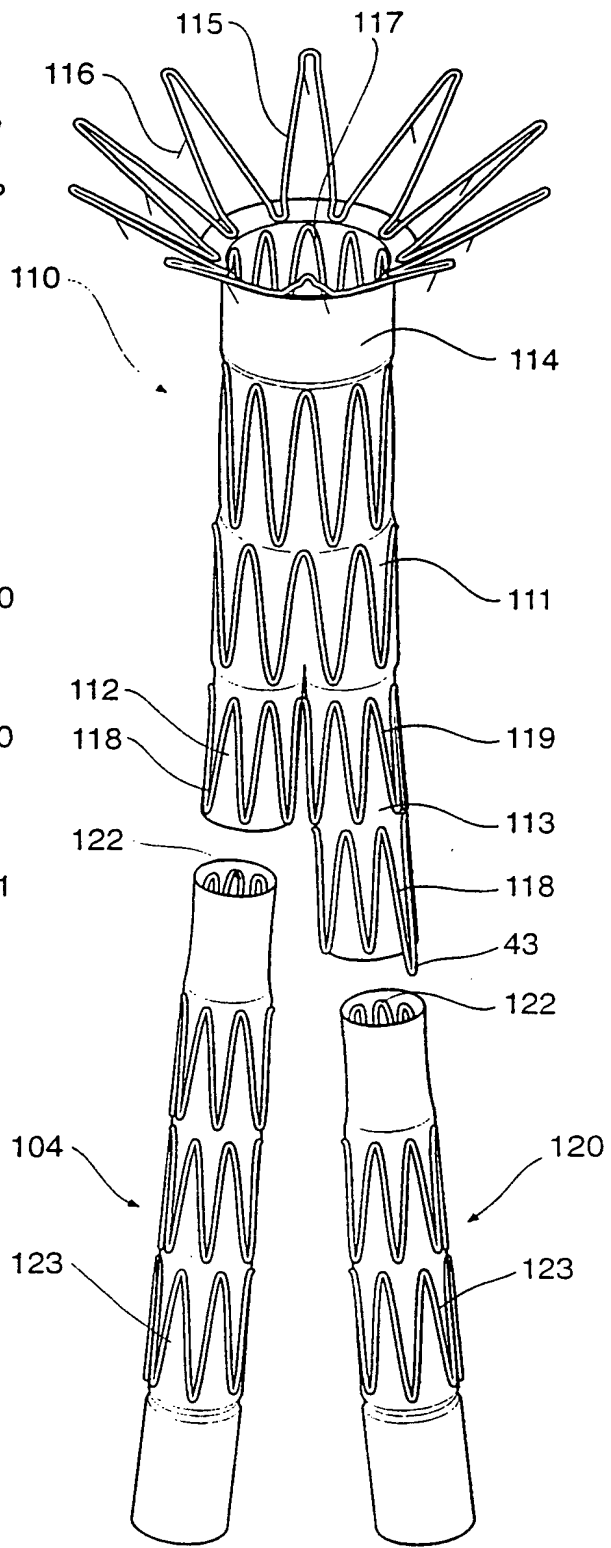


FIG 16

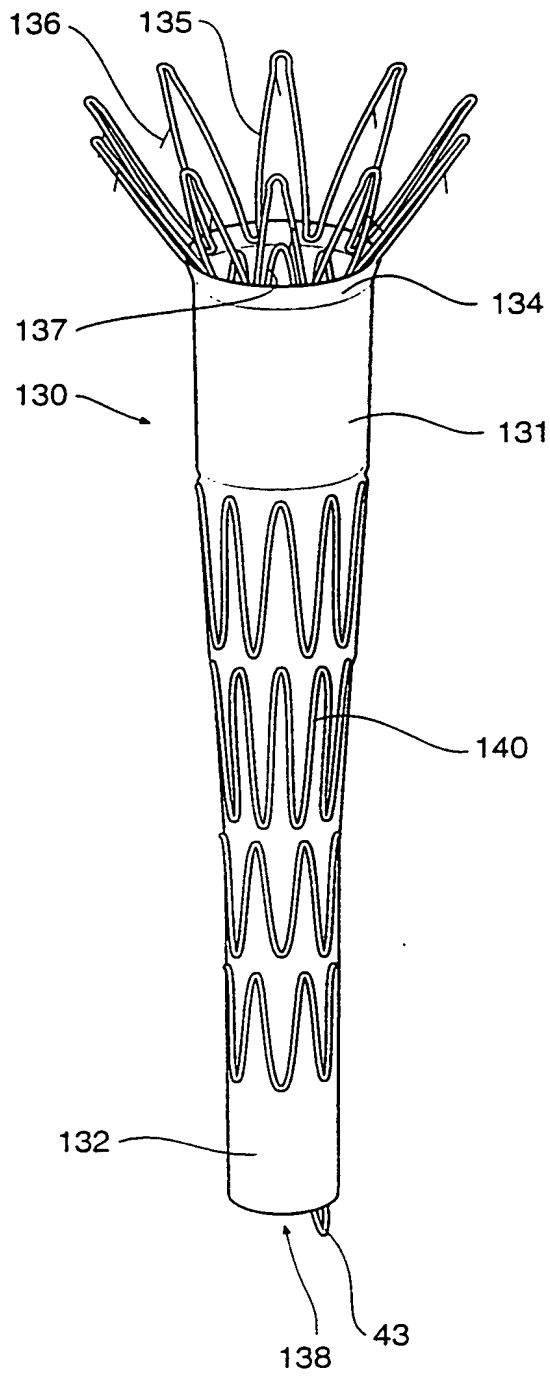


FIG 17

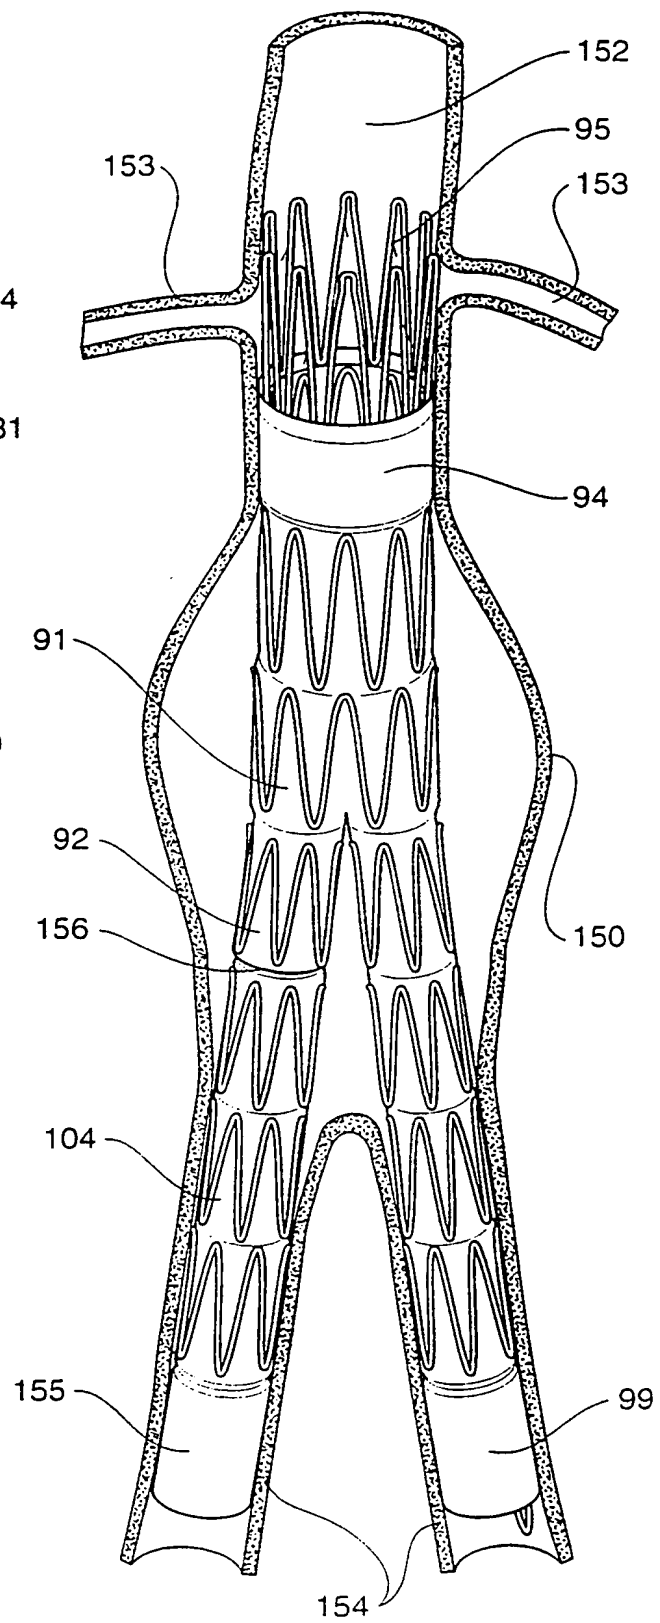


FIG 18